


Analysis heart rate data P.A. Tient

Nachtwacht LUNA software version 1.3


Bradycardie alarm between 5 and 40 BPM

General alarm below 5 and over 160 BPM


Labels	Values number of 2 second intervals	Average Heart Rate	Maximum Heartrate	Minimum Heartrate	Stdev of heartrate
30-4-2010	16546	66,4	146,0	41,0	8,3
no alarm	16546	66,4	146,0	41,0	8,3
1-5-2010	15211	68,8	104,0	41,0	8,5
no alarm	15211	68,8	104,0	41,0	8,5
2-5-2010	18884	68,0	108,0	37,0	9,1
no alarm	18884	68,0	108,0	37,0	9,1
3-5-2010	14559	64,9	111,0	31,0	8,4
no alarm	14552	64,9	111,0	31,0	8,4
Bradycardia	7	39,6	42,0	35,0	2,6
Total	65200	67,1	146,0	31,0	8,7

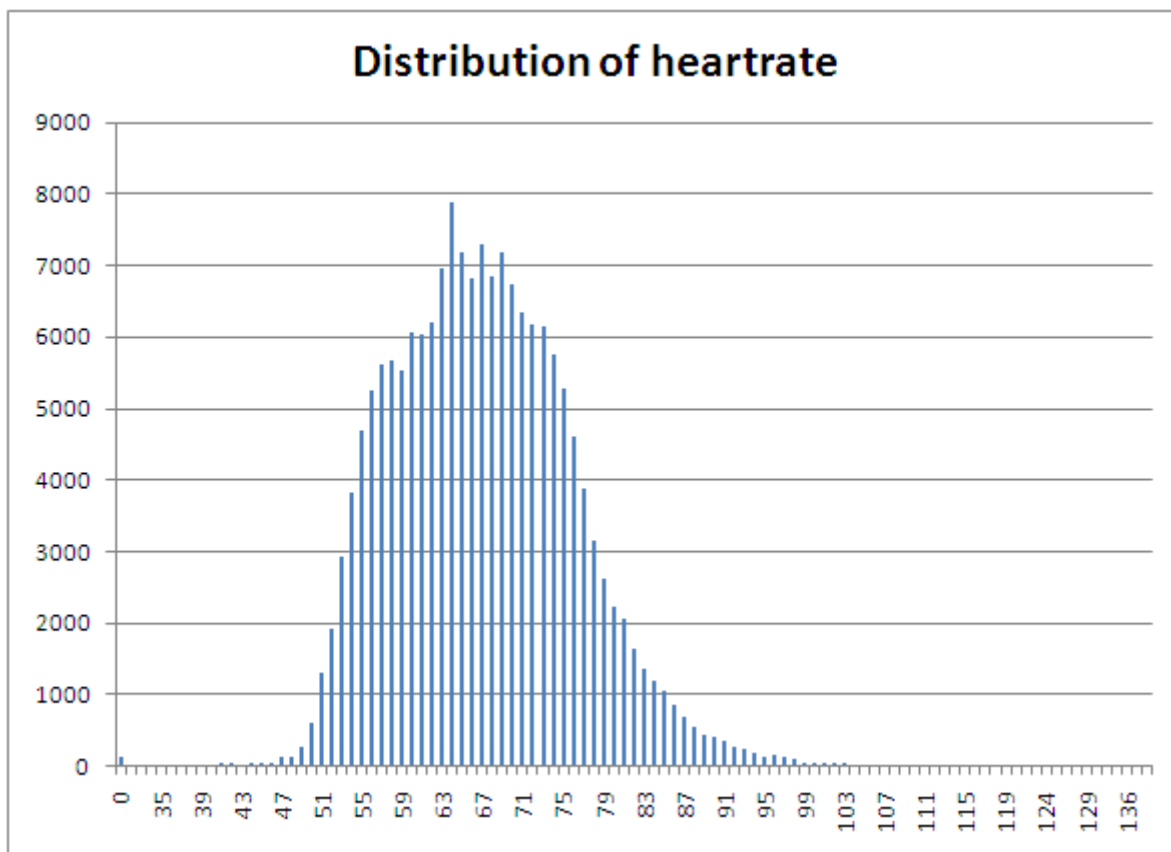


April 30 2010 – no alarm

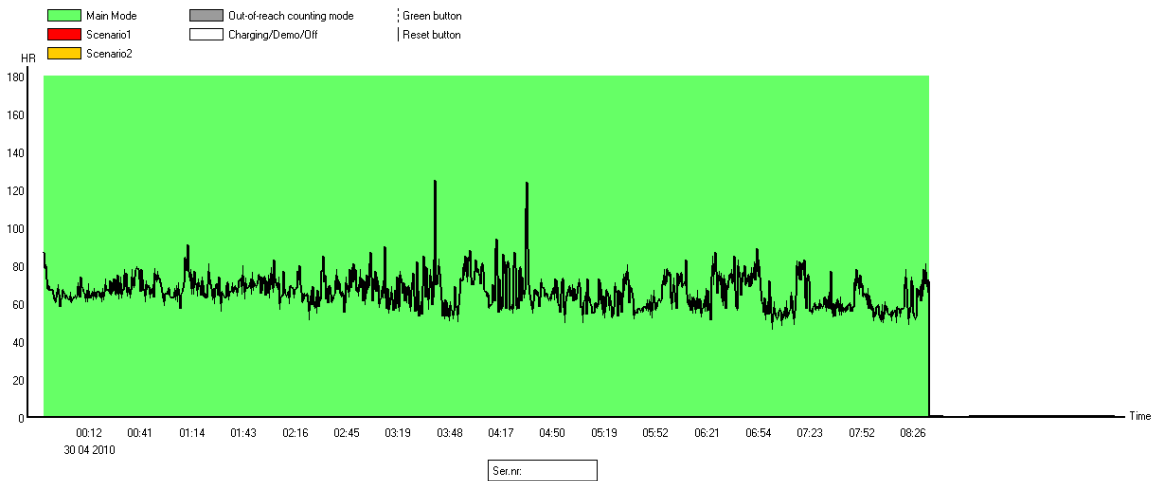


May 1, 2010 – geen alarm

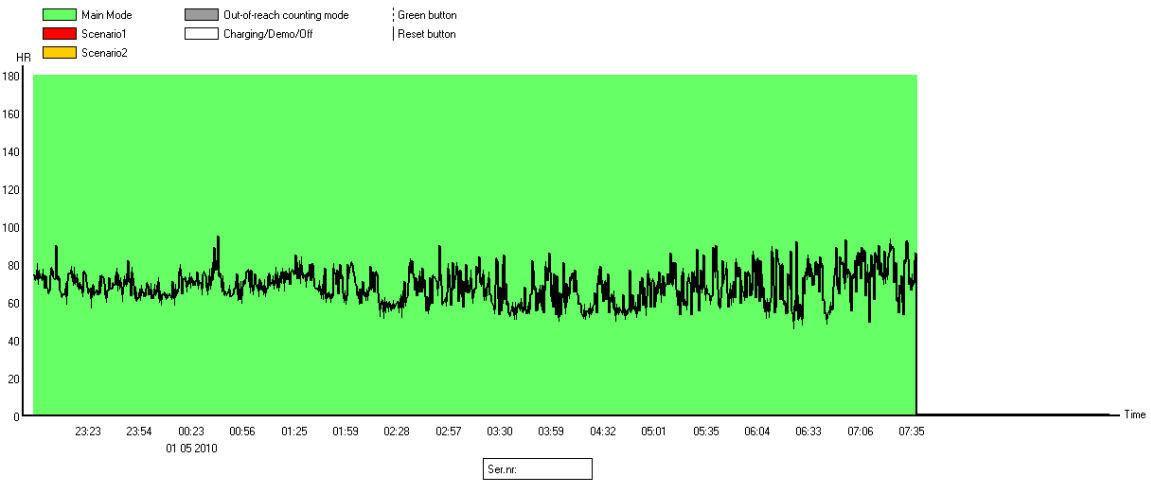


May 2, 2010 – geen alarm

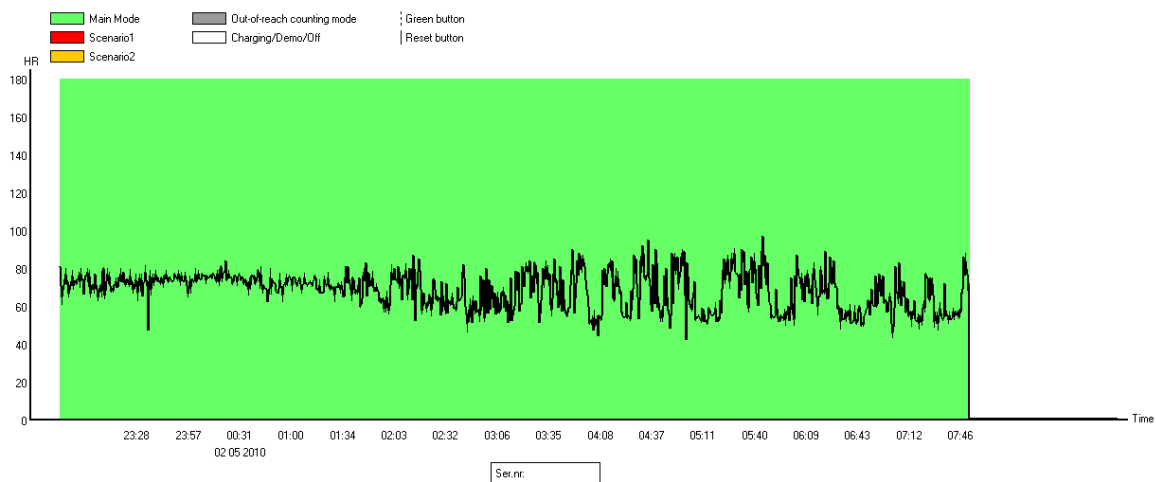

May 3, 2010 – no alarm, 1 warning for tachycardia

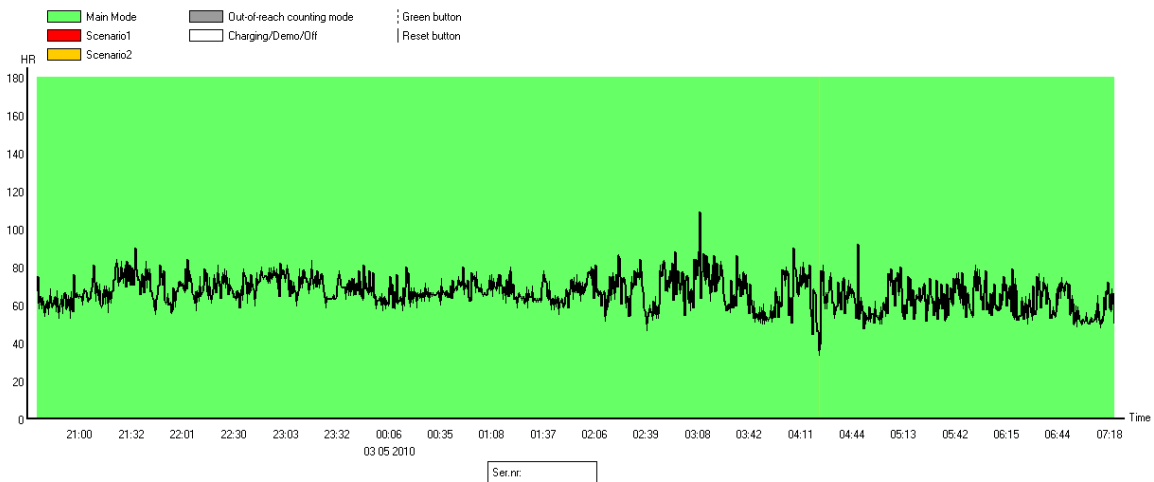

Zoomed in around 4:15 AM.

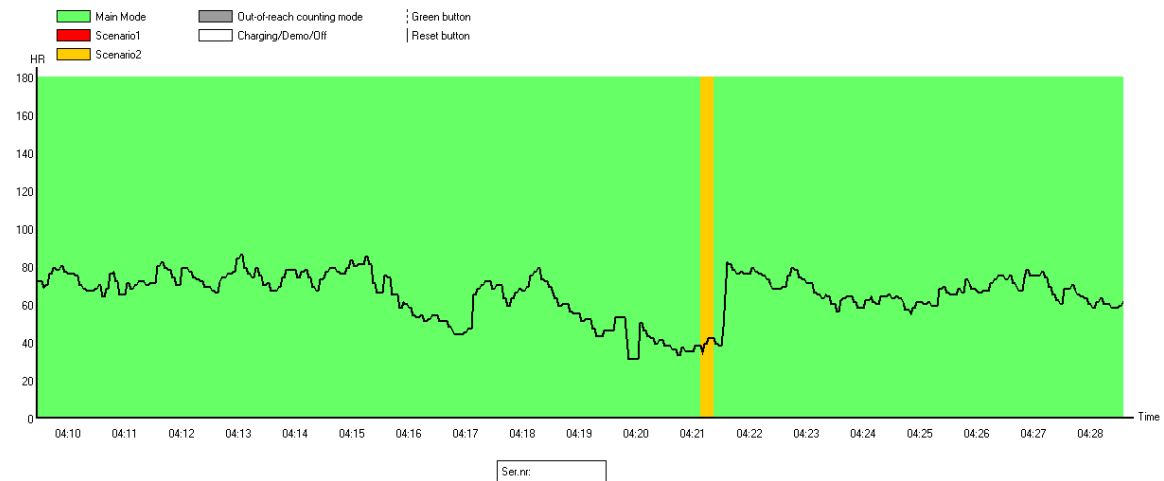

A possible Bradycardia deflected through a warning, after which the patient has recovered.

T.E. Stanalyst

Data analysis DAY4LIFE

+31 (0)40 - 29 13510

info@day4life.com